

Shake no more
All-in-one

free from manual shaking



01
Free from
Physical burden

Set then press a button

No need to shake a container for a given amount of time with force.

Safe measuring environment


No accidents caused by the unit slipping from your hands while shaking.



02
Free from
Inconsistent measurement value

Consistent measurement results regardless of measurement taker

Compared to the "manual shaking" method, measurement results from an automatic measurement will not be affected by the measurement taker.



03
Free from
Cumbersome operation

No cumbersome calculation after measurement

Using the preexisting and current data obtained by CooRe, a calibration curve can be created which can then be used to program a coefficient. Measurement values are automatically computed based off the past data, which means no stored data is wasted.

End User Feedback


~Company "S" Quality Assurance Department~

Unlike traditional instruments, it does not require intensive swinging motions, instead it can be readily used.

~Company "I" Product Development Department~

There is no more variation in measurement values that depend on who is measuring the sample.

Name of Compartment

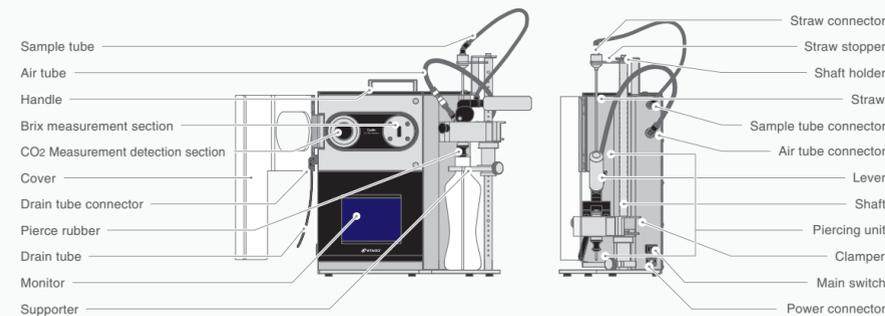

Specifications

Cat.No.	9332	9334
Model	CooRe	CooRe 3L
Measurement Scales	Brix (Automatic temperature compensation) CO ₂ Concentration (Automatic temperature compensation) Pressure Temperature	
Measurement System	Brix : Refractive index method CO ₂ Concentration : Converted from pressure Pressure : Sample agitation measurement method	
Measurement Range	Brix : 0.00 to 20.00 % CO ₂ Concentration : 0.000 to 12.000 vol. 0.000 to 24.000 × 10 ⁻⁶ kg/cm ³ 0.000 to 24.000 g/L Pressure : 0.00 to 10.00 bar 10 to 10000 mbar 0.000 to 145.000 psi 0.000 to 1.000 MPa 0 to 1000 kPa Temperature : 0.0 to 30.0 °C 32.0 to 86.0 °F 273 to 303 K	
Resolution	Brix : 0.01 % CO ₂ Concentration : 0.001 vol. 0.001 × 10 ⁻⁶ kg/cm ³ 0.001 g/L Pressure : 0.01 bar 10 mbar 0.001 psi 0.001 MPa 1 kPa Temperature : 0.1 °C 0.1 °F 1 K	
Measurement Accuracy	Brix (Absolute value) : ±0.05 % Pressure : ±1.0 % (at F.S. 20 °C) Temperature : ±1 °C	

Temperature	Brix	: 5.0 to 30.0 °C
Compensation Range	CO ₂ Concentration	: 0 to 25 °C
Minimum Sample Volume	Approx. 100 mL *1st measurement 200mL (Pressure chamber volume : 20mL)	
Data Display History	· Number · Measurement year month date time · Scale · Brix · Temperature when Brix is measured · CO ₂ concentration · Temperature when CO ₂ concentration is measured · Pressure · Temperature when pressure is measured	

Output	USB memory (CSV text file format)	
Pressure Resistance	Pressure chamber	: 1MPa
	Prism	: 1MPa
International Protection Class	IP65 *Applicable only if the USB terminal cover is on and power terminal cover is on (or AC power is connected).	
Power Supply	AC 100 to 240 V ,50/60Hz	
Power Consumption	70 VA	
Dimensions & Weight	CooRe	Approx. 40.5 × 21 × 45 cm 29lbs/13kg (Power cable included.)
	CooRe 3L	Approx. 40.5 × 21 × 51.5 cm 29lbs/13kg (Power cable included.)


Content

1. Main unit	1
2. Straw (with straw stopper and straw connector)	1
3. Extension Drain Tube	1
4. Connector (for Extension Drain Tube)	1
5. Shaft Lubricant for CooRe	1
6. AC power cable	1
7. Instruction manual	1
8. Inspection certificate	1

Accessories

Part Name	Part No.
Lithium-ion Battery	RE-74840
Pulp Filter Unit	RE-79424
Filter Cartridge (for Pulp Filter Unit)	RE-79425
Desiccant (100g)	RE-99440
Screw set for Back Cover	RE-99441
Extension Drain Tube	RE-78068
Shaft Lubricant for CooRe	RE-99442

Dimensions

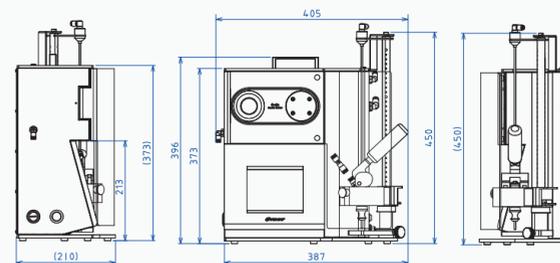

All ATAGO products are designed and manufactured in Japan.

ATAGO CO., LTD.

http://www.atago.net/ overseas@atago.net

ATAGO U.S.A., Inc. TEL : 1-425-637-2107
ATAGO INDIA Instruments Pvt. Ltd. TEL : 91-22-28544915, 40713232
ATAGO THAILAND Co., Ltd. TEL : 66-21948727-9
ATAGO BRASIL Ltda. TEL : 55 16 3913-8400
ATAGO ITALIA s. r. l. TEL : 39 02 36557267
ATAGO CHINA Guangzhou Co., Ltd. TEL : 86-20-38108256
ATAGO RUSSIA Ltd. TEL : 7-812-777-96-96
ATAGO NIGERIA Scientific Co., Ltd. TEL : 234-707-558-1552
ATAGO KAZAKHSTAN Ltd. TEL : 7-727-257-08-95

customer-service@atago-usa.com

customer-service@atago-india.com

customer-service@atago-thailand.com

customer-service@atago-brazil.com

customer-service@atago-italia.com

info@atago-china.com

info@atago-russia.com

atagonigeria@atago.net

info@atago-kazakhstan.com



ATAGO products comply with HACCP, GMP, and GLP system standards.

* Specifications and appearance are subject to change without notice.

Copyright © 2019 ATAGO CO., LTD. All rights reserved. ENV.04 1906800PP Printed in Japan

ATAGO®

Automatic CO₂ Brix Monitor

CO₂ Brix
CooRe
Portable Automatic Gas Volume Meter




CO₂ Brix Press a button. Simultaneous measurement.

Refractometer technology that ATAGO has cultivated for many years is incorporated into this gas volume meter. Two types of measurements can be taken at once, which improves work efficacy.



CooRe
CO₂ Brix Monitor

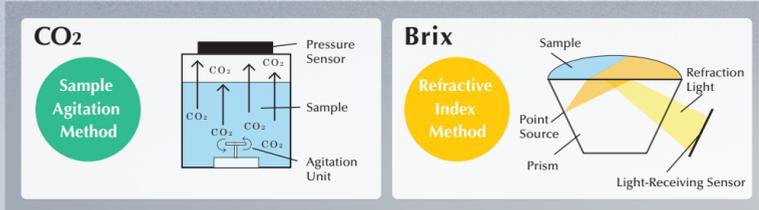

CooRe = Coo — Signifies CO₂ gas volume meter Re — Refractometer abbreviated

Readily take measurements any time, anywhere

No other automatic gas volume meter allows taking measurements any time and anywhere. CooRe is equipped with many convenient functions and components.

World first all-in-one piercing and measuring instrument

The piercing and measuring sections are together in one unit. Traditional automatic gas volume meters are equipped with nitrogen gas cylinders which weigh almost 10kg/22lbs. With CooRe, the pump is internalized requiring no need to connect or change the nitrogen gas cylinder.

Excellent operability

Easy piercing

This instrument can pierce any type of bottle easily and smoothly, whether can or bottle. In addition, it is equipped with a cover to prevent liquid from scattering when a bottle is removed from the instrument.

Sample amount is 100mL

Only 100mL of sample is required for measurements. If the capacity is that of the common soda bottle, all containers can be measured. *1st measurement 200mL

Cover

Cover to prevent liquid or pieces of a damaged can, glass bottle, or PET bottle from scattering.



Portable

Can be carried with one hand

The unit approximately weighs 13kg/29lbs. The weight being about half of traditional automatic gas volume meters, it is very easy to handle. The display and measurement sections are all in one place with a handle on the top to free up one of your hands during transit.



Can be used in area with no power supply

The power source can either be AC adapter or lithium ion battery. No more thinking about where to measure. Moreover, the rechargeable lithium ion battery can be used repeatedly, reducing running costs.

One minute to measure

After pressing the button, the measurement will automatically display in one minute. *1st measurement approx. 110 seconds


ATAGO's Reliability

ATAGO is a Brix meter manufacturer since 1940 serving 154 countries worldwide.




Touchscreen

Smooth and absolute operation

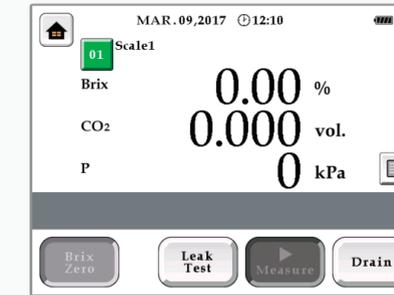

Measurement Screen


Before taking a measurement, select "LEAK TEST" then press "OK" once the completion message is displayed. Next, press "MEASURE" to begin taking measurements.

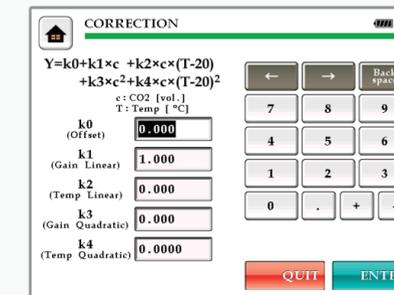

Value Correction Input Screen


Offset feature

Using the preexisting and current data obtained by CooRe, a calibration curve can be created which can then be used to program a coefficient. Measurement values are automatically computed based off of past data, which means no stored data is wasted.




Scale List Screen

By programming the scale, there is no need to reset the unit or mode.



Rinse Screen

Use this screen when rinsing at the beginning of the day or after the last use.



Data History Screen


Quickly access the last 500 measurements. With a touch, the measurements can be saved on a USB.




Settings Screen

Gateway to access basic configuration settings. Navigate to each configuration page using the icons. Confusion-free, intuitive operation.


Measurement Method




Step1 **Set** a sample



Step2 **Pull down** the lever



Step3 **Press** Measure button

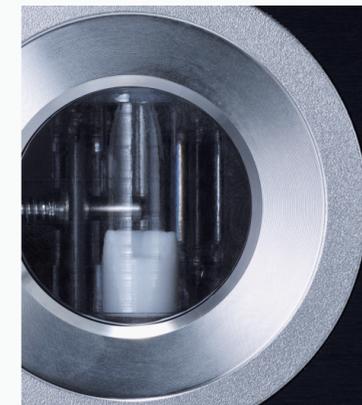

CooRe
CO₂ Brix Monitor